
Cardiac Arrest (CA)
Event Button (EB)
Name: [redacted]
Date: 08/17/2020
Time: 08:17:59
Duration: 00:00:30
Low Alarm: 50 bpm
High Alarm: 120 bpm
Alarm Delay: 10 sec
Min: 76 Max: 76 Avg: 76
Total Beats: 38
Ventricular Ectopics: 0
Supraventricular Ectopics: 0
Pauses: 0
Longest Pause: 0.00 sec
Couplets: 0
Runs: 0
Longest Run: 0 beats
Fastest Run: 0 bpm
Fastest Beat: 76 bpm
Slowest Run: 0 bpm
Slowest Beat: 76 bpm
Max Heart Rate: 76 bpm
Min Heart Rate: 76 bpm
Mean Heart Rate: 76 bpm
Heart Rate Variability: 0.00
Patient Events: 0
Technician Events: 0
Triggered Events: 0
Manual Events: 0
Ventricular Ectopic Beats
Supraventricular Ectopic Beats
Pauses
Couplets
Runs
Patient Events
Technician Events
Triggered Events
Manual Events
Recorded by a Lifewatch device
Reviewed by
Comments
Page 1 of 1
Lifewatch Technologies Ltd. 2020
Lifewatch Technologies Ltd. 2020
Lifewatch Technologies Ltd. 2020

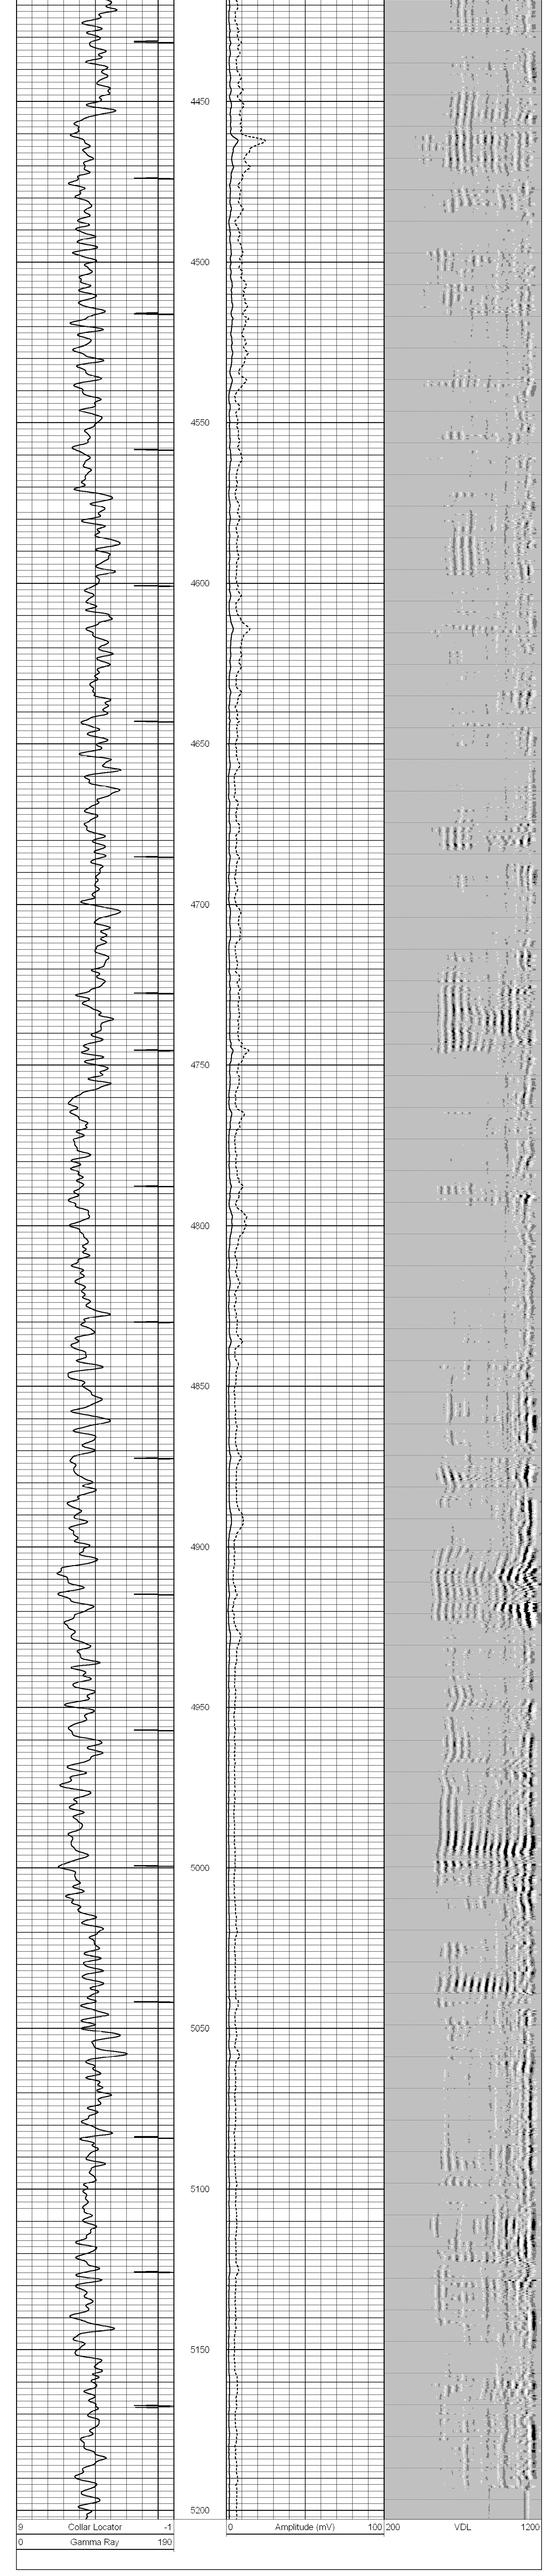
4450
4500
4550
4600
4650
4700
4750
4800
4850
4900
4950
5000
5050
5100
5150
5200
9
Collar Locator
-1
0
Gamma Ray
190
0
Amplitude (mV)
100
200
VDL
1200