


# Data Collection Report

Stitt Gas Unit #2 MIT test

Gauge Information	
Serial Number	358534
Model	10KPSIXP2I
Message Store	
Units	PSI

Run Info	
Start Time	7/17/17 2:45:00 PM
Stop Time	7/17/17 3:01:01 PM
Logging Interval	30

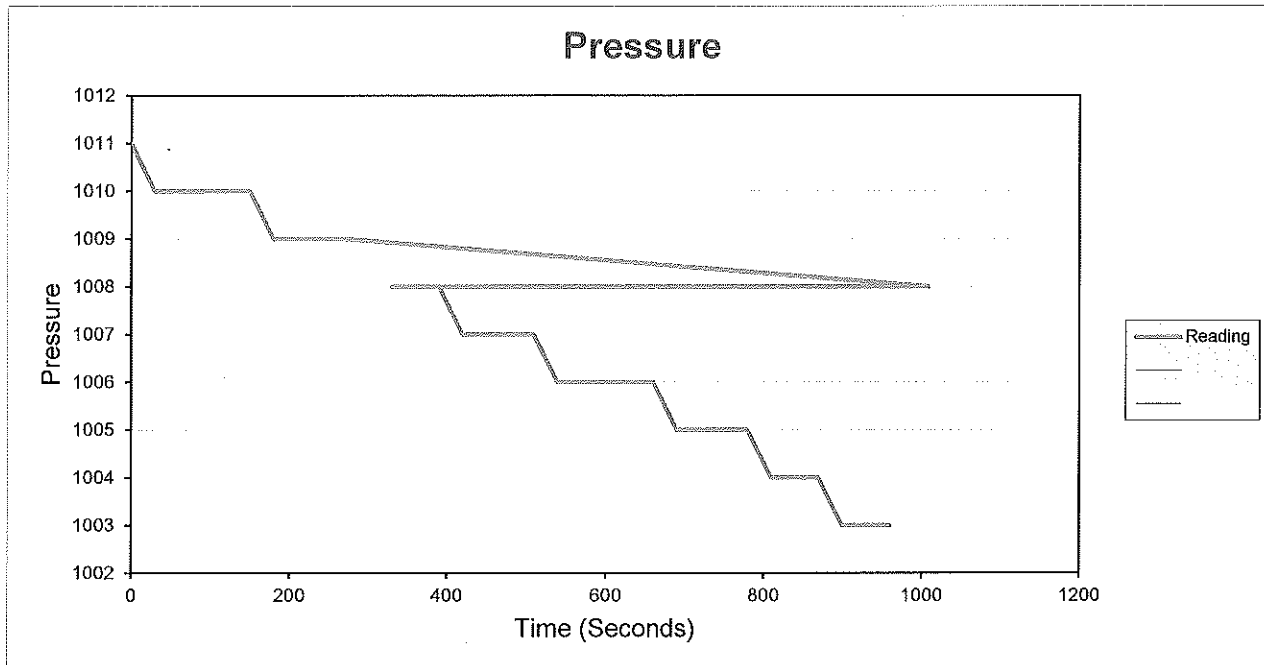

Serial Number 358534  
 Model 10KPSIXP2I  
 Units PSI  
 Firmware Version R0224      Message Store -----  
 Run Index 1  
 Logging Type Actual  
 Logging Interval 30  
 Start Time 7/17/2017 14:45  
 Stop Time 7/17/2017 15:01  
 Time Reading

Event      Event Data  
 Battery OK  
 Logging Interval, 30  
 Tare, 0

0	1011
30	1010
60	1010
90	1010
120	1010
150	1010
180	1009
210	1009
240	1009
270	1009
1008	1008
330	1008
360	1008
390	1008
420	1007
450	1007
480	1007
510	1007
540	1006
570	1006
600	1006
630	1006
660	1006
690	1005
720	1005
750	1005
780	1005
810	1004
840	1004
870	1004
900	1003
930	1003
960	1003