

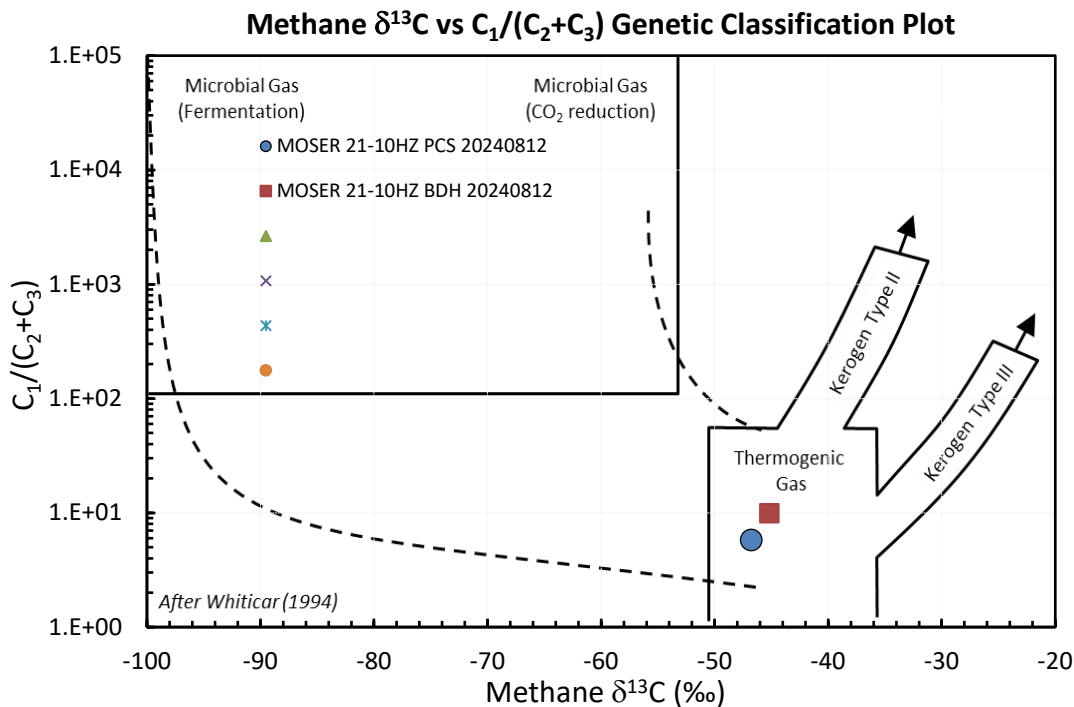
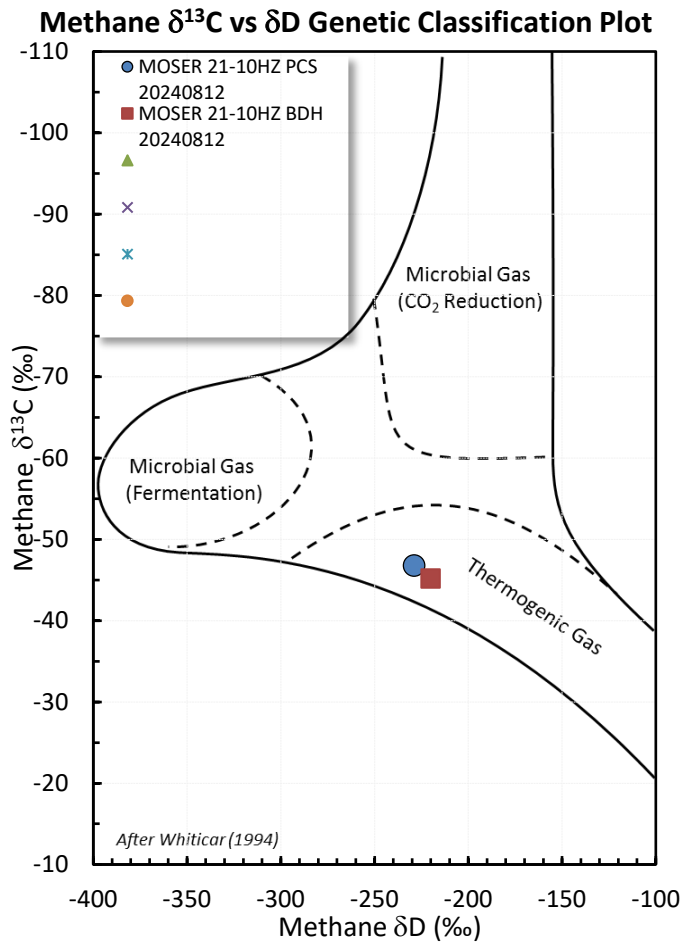


Stable Isotope Interpretive Plots

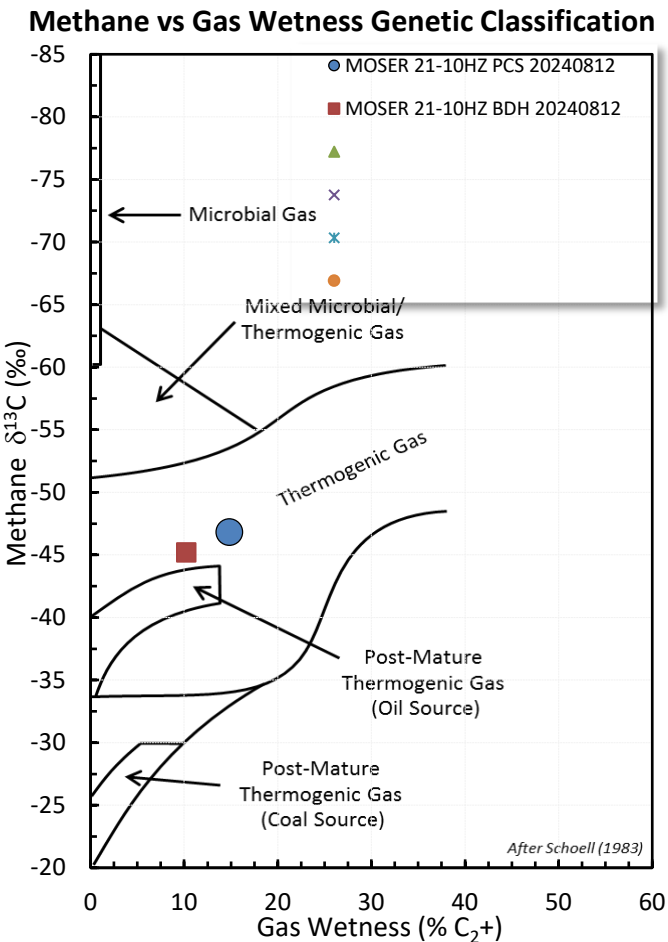

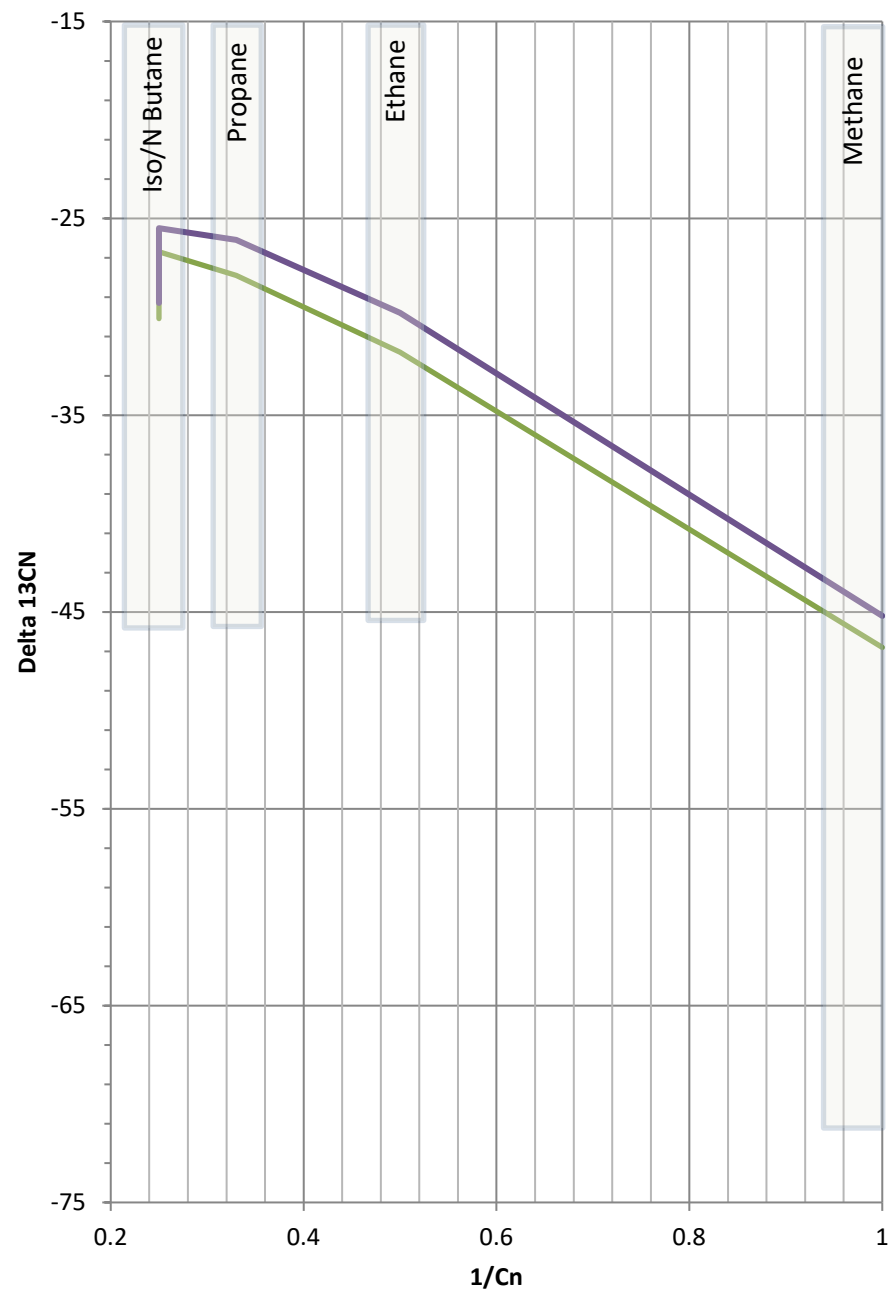

MOSER 21-10HZ PCS

MOSER 21-10HZ BDH

Bradenhead Test Summary

