


Site Information	
Site Name	Herman 632-14
Date	04/28/2005
Sampler	Kendra Correy
Weather	70° sunny

Gas Meter Information	
Make/Model	GEM 5000
S/N	5071

Calibration Information	
Gas	Time
Pure N ₂	1354
Fresh Air	1352
50 ppm CO, 10 ppm H ₂ S	1356
15% CH ₄ , 15% CO ₂ , Bal N ₂	1357

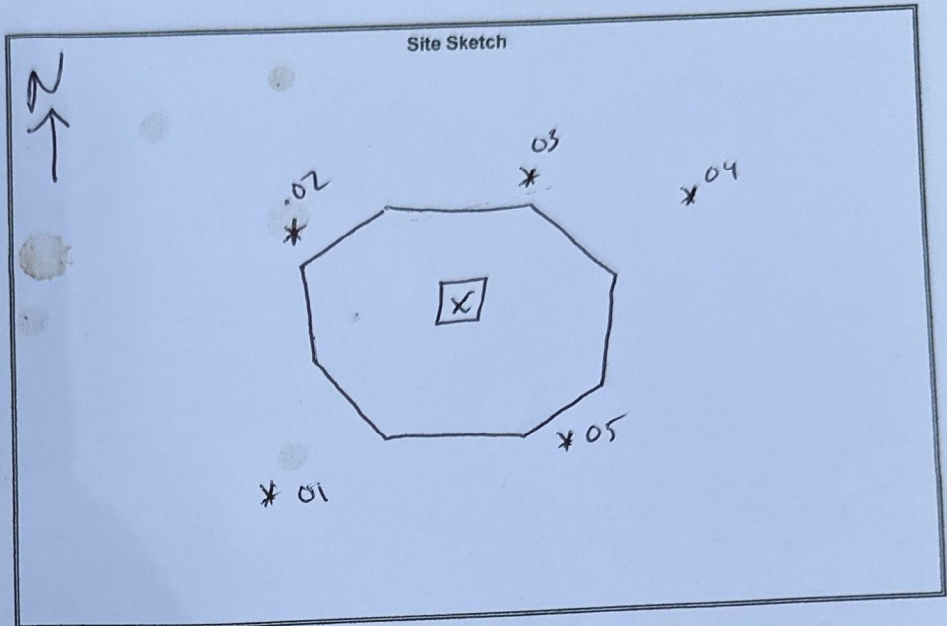

Bump Test						
Time		CH ₄ (%)	CO ₂ (%)	O ₂ (%)	H ₂ S (ppm)	CO (ppm)
1400	Calibration Gas	15.0	15.0	0.0	0	0
	Readings	14.9	15.0	0.0	0	0

Field Readings										
Point ID	Time	CH ₄ (%)	CO ₂ (%)	O ₂ (%)	H ₂ S (ppm)	CO (ppm)	Purge Length	Sampled? (Y/N)	Sample ID	Comments
SV01										Blocked
SV02										Blocked
SV03	1429	0.0	0.1	19.9	0	0	63			CO to 51
SV04	1431	0.0	0.1	19.9	0	0	61			CO to 20
SV05										Blocked

Notes and Observations