

Stage 2 Data Validation Memorandum
Chevron Bishop Loss of Containment Response Site
Galeton, Colorado
Solid Samples
Sample Delivery Group: L1853786
Report Date: June 2, 2025

This quality assurance (QA) review is based upon an examination of the data generated from the analyses of the four solid samples and associated quality control (QC) samples (including aqueous blanks) collected on April 30, 2025, at the Chevron Bishop Loss of Containment Response Site in Galeton, Colorado. These samples were collectively analyzed by Pace Analytical National Center for Testing and Innovation (Pace National) of Mount Juliet, Tennessee, for volatile organic compounds (VOCs) by SW-846 Method 8260D, semivolatiles organic compounds (SVOCs) by SW-846 Method 8270E, total metals by SW-846 Methods 6010D, nitrate-nitrite by SW-846 Method 9056A, ammonia nitrogen by US EPA Method 350.1, total nitrogen by calculation, total Kjeldahl nitrogen (TKN) by SM 4500-NORG-C, and total organic carbon (TOC) by American Society of Agronomy (ASA) Walkley-Black method.

This review was performed in accordance with the Bishop Loss of Containment, Galeton, Colorado Environmental Sampling and Analysis Plan (CTEH; Version 1.4, May 7, 2025), the Bishop Loss of Containment Incident Draft Quality Assurance Project Plan (QAPP; Environmental Standards, Inc. [Environmental Standards]; Version 1.0, April 25, 2025), and the above-referenced analytical methods. This review was performed with guidance from the National Functional Guidelines for Organic Superfund Methods Data Review (US EPA, 2020) and the National Functional Guidelines for Inorganic Superfund Methods Data Review (US EPA, 2020). These validation guidance documents specifically address analyses performed in accordance with the CLP analytical methods and are not completely applicable to the type of analyses and analytical protocols performed for the SM, SW-846, US EPA, and ASA methods utilized by the laboratory for these samples. Environmental Standards used professional judgment to determine the quality of the analytical results and compliance relative to the SM, SW-846, US EPA, and ASA methods utilized by the laboratory.

Summary

The analytical results and associated laboratory QC samples were reviewed to determine the integrity of the reported analytical results and to ensure that the data met the established measurement quality objectives. This QA review includes all samples in Pace National Sample Delivery Group (SDG) L1853786.

The samples that have undergone Stage 2 data validation are listed below:

Sample Identification	Laboratory Sample Identification	Laboratory SDG	Matrix	Date Sample Collected	Parameter(s) Examined
GACO0430T031S007	L1853786-01	L1853786	Solid	4/30/25	VOC, SVOC, TPH, DRO, M, Hg, Cr6
GACO0430T031S006	L1853786-02	L1853786	Solid	4/30/25	VOC, SVOC, TPH, DRO, M, Hg, Cr6, N+N, NH ₃ , TN, TKN, TOC
GACO0430T031S005	L1853786-03	L1853786	Solid	4/30/25	VOC, SVOC, TPH, DRO, M, Hg, Cr6
GACO0430T031T002 (Trip Blank)	L1853786-04	L1853786	Aq	4/30/25	VOC

Notes:

- VOC - VOCs by SW-846 Method 8260D.
- SVOC - SVOCs by SW-846 Method 8270E.
- M - Total Metals by SW-846 Method 6010D.
- N+N - Nitrate-Nitrite by SW-846 Method 9056A.
- NH₃ - Ammonia Nitrogen by US EPA Method 350.1
- TN - Total Nitrogen by Calculation.
- TKN - TKN by SM 4500-NORG-C.
- TOC - TOC by ASA Walkley-Black Method.
- Aq - Aqueous.



ITEMS REVIEWED

Chain-of-Custody (COC) Record and Case Narrative	Sample Preservation and Condition Upon Laboratory Receipt
Holding Times	Surrogate Recovery
Blank Results	Laboratory Results
Laboratory Control Sample (LCS) Results	Matrix Spike and Matrix Spike Duplicate (MS/MSD) Results
Results Reported Between the Method Detection Limit (MDL)/Reporting Limit (RL) and Quantitation Limit (QL)	Percent Solids

Comments

1. The analysis for 1,2-dichloroethane in GACO0430T031T002 should be considered unusable due to very low (<10%) LCS/LCSD recoveries. The result that has been flagged "R" is addressed on the table below.
2. The analysis for hexachlorocyclopentadiene in GACO0430T031S007 should be considered unusable due to very low (<10%) LCS/LCSD recoveries. The result that has been flagged "R" is addressed on the table below.

Based on the items included in this QA review, the following qualifiers are offered.

Analyte(s)	Sample(s)	Validation Qualifier	Reason(s) for Qualification
1,2-dichloroethane	GACO0430T031T002	R	LC-
hexachlorocyclopentadiene	GACO0430T031S007	R	MS-
aluminum	all samples	J	MS, MSP
iron and manganese	all samples	J-	MS-

- All positive results reported between the MDL/RL and QL should be considered estimated and have been flagged "J" on the data tables. (Reason Code RL)
- When sample results were qualified both as estimated with a direction of bias ("J+" or "J-") and as estimated with unknown bias ("J") or the opposite bias, only the unknown bias qualifier has been included on the data tables.

Review performed by: Amanda Williams, Quality Assurance Chemist
 Report reviewed by: Bryan J. Eck, Project Quality Assurance Chemist
 Report approved by: Amanda J. Cover, CEAC, Associate Chemist/Project Manager
 Date review completed: 6/2/2025

SECTION 2

ANALYTICAL RESULTS

DATA QUALIFIERS

- U** The analyte was analyzed for, but was not detected above the level of the adjusted detection limit or quantitation limit, as appropriate.
- R** The data are unusable. The sample results are rejected due to serious deficiencies in meeting QC criteria. The analyte may or may not be present in the sample.
- J** The result is an estimated quantity. The associated numerical value is the approximate concentration of the analyte in the sample.
- J+** The result is an estimated quantity, but the result may be biased high.
- J-** The result is an estimated quantity, but the result may be biased low.
- UJ** The analyte was analyzed for but was not detected. The reported quantitation limit is approximate and may be inaccurate or imprecise.
- NJ** The analyte has been “tentatively identified” or “presumptively” as present and the associated numerical value is the estimated concentration in the sample.




REASON CODES AND EXPLANATIONS

Reason Code ¹	Description
¹ For any Reason Code that does not indicate that the potential bias is indeterminate, the "+" or "-" reason code may be appended to the qualification reason code in order to indicate a direction of bias (e.g., MS+ would be used to indicate potential high bias due to a high matrix spike recovery)	
+	The associated quality control item indicates a potential high bias in the sample result
-	The associated quality control item indicates a potential low bias in the sample result
AST	Compound not quantitated against an authentic standard; potential bias indeterminate
BF	Contamination present in a field blank (e.g., Field Blank, Equipment Blank, etc.); evaluation criteria exceeded
BL	Contamination present in a laboratory blank (e.g., Method Blank, Instrument Blank, etc.); evaluation criteria exceeded
BN	Elevated detection limit or estimated result due to negative instrument drift (e.g., negative instrument blank result with an absolute value > 2× the method detection limit)
BT	Contamination present in the Trip Blank; evaluation criteria exceeded
CC	Possible contamination due to carryover from a previous sample
CR	Calculated result in which one or more of the components has been qualified
CRQ	Calculated result flagged due to reporting protocol
CT	Cooler temperature criteria not met
CV	Continuing calibration verification evaluation criteria not met
CY	Chemical Yield recovery criteria not met
DI	Detector instability (radionuclide chemistry); potential bias indeterminate
EC	Result exceeds the calibration range; potential bias indeterminate
FD	Field duplicate imprecision; potential bias indeterminate
FP	Target compound identification criteria not met; potential false positive
GH	Headspace present in the gamma spectrometer sample analysis vessel; potential bias indeterminate
GS	Low sample density in the gamma spectrometer sample analysis vessel; potential bias indeterminate
HT	Holding time exceeded
HV	Headspace present in volatile vials
IC	Initial calibration evaluation criteria not met

Reason Code ¹	Description
IN	Interference (e.g., laboratory, chemical, chromatographic/instrumental, and/or matrix) present in the analysis
IR	Interference check standard evaluation criteria not met
IS	Internal standard evaluation criteria not met
LC	Laboratory control sample/laboratory control sample duplicate recovery criteria not met
LCP	Laboratory control sample/laboratory control sample duplicate precision criteria not met; potential bias indeterminate
LD	Laboratory duplicate precision criteria not met; potential bias indeterminate
LR	Linear range exceeded; potential bias indeterminate
MDP	Laboratory deviated from the method for a method-defined parameter, based on regulatory requirements
MS	Matrix spike/matrix spike duplicate recovery criteria not met
MSP	Matrix spike/matrix spike duplicate precision criteria not met; potential bias indeterminate
NQC	Absence of supporting quality control samples
PD	Post-digestion spike recovery criteria not met
OT	Other deficiencies, see validation report for additional details
PM	Performance evaluation mixture criteria not met
PS	Low percent solids; potential bias indeterminate
PT	Chromatographic pattern in sample does not match pattern of calibration standard
QCI	Quantitation/confirmation ion ratios in sample are inconsistent with reference spectra; potential bias indeterminate
RA	Replicate/multiple analyses criteria not met; potential bias indeterminate
RM	Reference material recovery criteria not met
RL	The analysis meets all qualitative identification criteria, but the measured concentration is between the method detection limit and the quantitation or reporting limit; potential bias indeterminate
RS	Reporting limit standard(s) outside of acceptance limits
SA	Method of standard additions criteria not met; potential bias indeterminate
SC	Relative percent difference between two columns exceeds criteria; potential bias indeterminate
SCC	Second column confirmation was not performed as required by the analysis method

Reason Code ¹	Description
SCT	Sample counting time error (radionuclide chemistry); potential bias indeterminate
SD	Serial dilution results did not meet evaluation criteria
SP	Sample preservation criteria not met
SR	Surrogate recovery criteria not met
SS	Second source calibration verification/initial calibration verification criteria not met
ST	Sample container type incorrect
SU	Sample result is less than the two-sigma uncertainty
SUN	Absolute value of the negative sample result is greater than the two-sigma uncertainty
SW	Sample switch suspected
TD	Result for dissolved constituent significantly exceeded result for total constituent; potential bias indeterminate
TIR	Tentatively identified compound; observed in an associated laboratory, equipment, field, or trip blank.
TN	Instrument tune criteria not met
Y	Potential bias due to the y-intercept in the calibration curve significantly affecting the analyte response

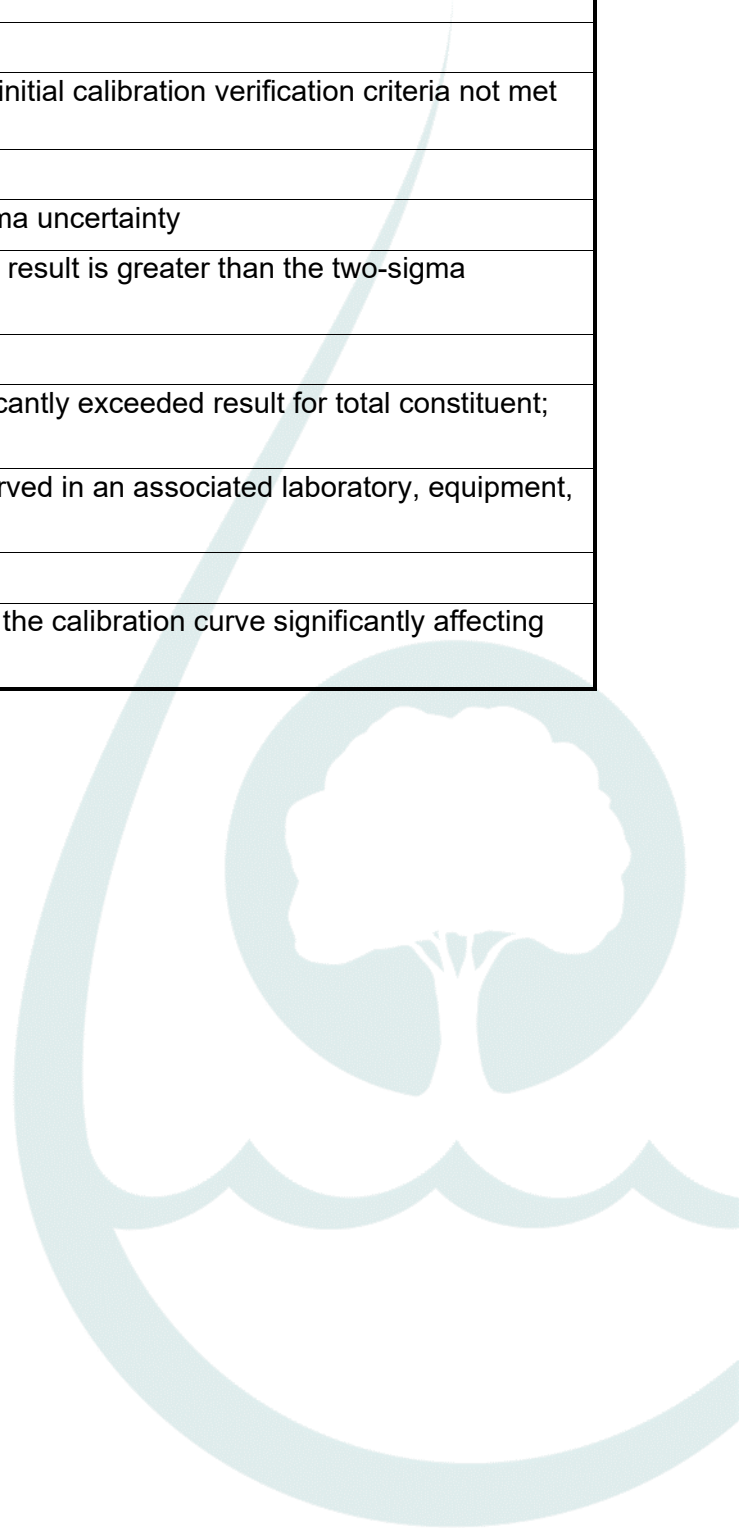

Lab Sample ID	L1853786-01
Sys Sample Code	GACO0430T031S007
Sample Name	GACO0430T031S007
Sample Date	4/30/2025 3:35:00 PM
Sample Type	N
Matrix	SO
Parent Sample	
% Moisture	14.20

Analytic Method	Chemical Name	CAS Rn	Fraction	Test Type	Result Unit	Final Result	Final Qual	Reason code	Final MDL	Final RL	Final QL	Final Detect	Final Report	DF	Basis
CALC	Total Nitrogen	TN	N	INITIAL	ug/Kg	2140000			706	706	23300	Y	Y	1	DRY
E350.1	Ammonia Nitrogen	7664-41-7	N	INITIAL	ug/Kg		U		8380	8380	11700	N	Y	1	DRY
SM2540G	Total Solids	10-31-1	N	INITIAL	%	85.8						Y	Y	1	NA
SM4500-NORG-D	Kjeldahl Nitrogen, TKN	7727-37-9TKN	N	INITIAL	ug/Kg	2080000			177000	177000	233000	Y	Y	10	DRY
SW6010	Aluminum	7429-90-5	T	INITIAL	ug/Kg	3140000	J	MS,MSP	7090	7090	23300	Y	Y	1	DRY
	Antimony	7440-36-0	T	INITIAL	ug/Kg		U		806	806	2330	N	Y	1	DRY
	Beryllium	7440-41-7	T	INITIAL	ug/Kg	561			55.6	55.6	233	Y	Y	1	DRY
	Calcium	7440-70-2	T	INITIAL	ug/Kg	8720000			22200	22200	117000	Y	Y	1	DRY
	Cobalt	7440-48-4	T	INITIAL	ug/Kg	4670			206	206	1170	Y	Y	1	DRY
	Iron	7439-89-6	T	INITIAL	ug/Kg	3860000	J-	MS-	2610	2610	11700	Y	Y	1	DRY
	Magnesium	7439-95-4	T	INITIAL	ug/Kg	2250000			23200	23200	117000	Y	Y	1	DRY
	Manganese	7439-96-5	T	INITIAL	ug/Kg	306000	J-	MS-	202	202	1170	Y	Y	1	DRY
	Potassium	7440-09-7	T	INITIAL	ug/Kg	2390000			24400	24400	117000	Y	Y	1	DRY
	Sodium	7440-23-5	T	INITIAL	ug/Kg	225000			48000	48000	117000	Y	Y	1	DRY
	Thallium	7440-28-0	T	INITIAL	ug/Kg		U		604	604	2330	N	Y	1	DRY
Vanadium	7440-62-2	T	INITIAL	ug/Kg	14700			447	447	2330	Y	Y	1	DRY	
SW8260	1,1,1,2-Tetrachloroethane	630-20-6	N	INITIAL	ug/Kg		U		1.26	1.26	3.33	N	Y	1	DRY
	1,1,1-Trichloroethane	71-55-6	N	INITIAL	ug/Kg		U		1.23	1.23	3.33	N	Y	1	DRY
	1,1,2,2-Tetrachloroethane	79-34-5	N	INITIAL	ug/Kg		U		0.926	0.926	3.33	N	Y	1	DRY
	1,1,2-Trichloroethane	79-00-5	N	INITIAL	ug/Kg		U		0.795	0.795	3.33	N	Y	1	DRY
	1,1,2-Trichlorotrifluoroethane	76-13-1	N	INITIAL	ug/Kg		U		1.00	1.00	3.33	N	Y	1	DRY
	1,1-Dichloroethane	75-34-3	N	INITIAL	ug/Kg		U		0.654	0.654	3.33	N	Y	1	DRY
	1,1-Dichloroethene	75-35-4	N	INITIAL	ug/Kg		U		0.807	0.807	3.33	N	Y	1	DRY
	1,1-Dichloropropene	563-58-6	N	INITIAL	ug/Kg		U		1.08	1.08	3.33	N	Y	1	DRY
	1,2,3-Trichlorobenzene	87-61-6	N	INITIAL	ug/Kg		U		9.76	9.76	16.6	N	Y	1	DRY
	1,2,3-Trichloropropane	96-18-4	N	INITIAL	ug/Kg		U		2.16	2.16	16.6	N	Y	1	DRY
	1,2,3-Trimethylbenzene	526-73-8	N	INITIAL	ug/Kg		U		2.10	2.10	6.66	N	Y	1	DRY
	1,2,4-Trichlorobenzene	120-82-1	N	INITIAL	ug/Kg		U		5.86	5.86	16.6	N	Y	1	DRY
	1,2-Dibromo-3-Chloropropane	96-12-8	N	INITIAL	ug/Kg		U		5.19	5.19	33.3	N	Y	1	DRY
	1,2-Dibromoethane	106-93-4	N	INITIAL	ug/Kg		U		0.863	0.863	3.33	N	Y	1	DRY
	1,2-Dichlorobenzene	95-50-1	N	INITIAL	ug/Kg		U		0.566	0.566	6.66	N	Y	1	DRY
	1,2-Dichloroethane	107-06-2	N	INITIAL	ug/Kg		U		0.864	0.864	3.33	N	Y	1	DRY

Lab Sample ID	L1853786-01
Sys Sample Code	GACO0430T031S007
Sample Name	GACO0430T031S007
Sample Date	4/30/2025 3:35:00 PM
Sample Type	N
Matrix	SO
Parent Sample	
% Moisture	14.20

Analytic Method	Chemical Name	CAS Rn	Fraction	Test Type	Result Unit	Final Result	Final Qual	Reason code	Final MDL	Final RL	Final QL	Final Detect	Final Report	DF	Basis
SW8260	1,2-Dichloropropane	78-87-5	N	INITIAL	ug/Kg		U		1.89	1.89	6.66	N	Y	1	DRY
	1,3-Dichlorobenzene	541-73-1	N	INITIAL	ug/Kg		U		0.799	0.799	6.66	N	Y	1	DRY
	1,3-Dichloropropane	142-28-9	N	INITIAL	ug/Kg		U		0.667	0.667	6.66	N	Y	1	DRY
	1,4-Dichlorobenzene	106-46-7	N	INITIAL	ug/Kg		U		0.932	0.932	6.66	N	Y	1	DRY
	2,2-Dichloropropane	594-20-7	N	INITIAL	ug/Kg		U		1.84	1.84	3.33	N	Y	1	DRY
	2-Butanone (MEK)	78-93-3	N	INITIAL	ug/Kg		U		84.6	84.6	133	N	Y	1	DRY
	2-Chlorotoluene	95-49-8	N	INITIAL	ug/Kg		U		1.15	1.15	3.33	N	Y	1	DRY
	4-Chlorotoluene	106-43-4	N	INITIAL	ug/Kg		U		0.599	0.599	6.66	N	Y	1	DRY
	4-Methyl-2-pentanone (MIBK)	108-10-1	N	INITIAL	ug/Kg		U		3.04	3.04	33.3	N	Y	1	DRY
	Acetone	67-64-1	N	INITIAL	ug/Kg		U		48.6	48.6	66.6	N	Y	1	DRY
	Acrylonitrile	107-13-1	N	INITIAL	ug/Kg		U		4.81	4.81	16.6	N	Y	1	DRY
	Bromobenzene	108-86-1	N	INITIAL	ug/Kg		U		1.20	1.20	16.6	N	Y	1	DRY
	Bromodichloromethane	75-27-4	N	INITIAL	ug/Kg		U		0.966	0.966	3.33	N	Y	1	DRY
	Bromoform	75-25-2	N	INITIAL	ug/Kg		U		1.56	1.56	33.3	N	Y	1	DRY
	Bromomethane	74-83-9	N	INITIAL	ug/Kg		U		2.62	2.62	16.6	N	Y	1	DRY
	Carbon tetrachloride	56-23-5	N	INITIAL	ug/Kg		U		1.20	1.20	6.66	N	Y	1	DRY
	Chlorobenzene	108-90-7	N	INITIAL	ug/Kg		U		0.280	0.280	3.33	N	Y	1	DRY
	Chlorodibromomethane	124-48-1	N	INITIAL	ug/Kg		U		0.815	0.815	3.33	N	Y	1	DRY
	Chloroethane	75-00-3	N	INITIAL	ug/Kg		U		2.26	2.26	6.66	N	Y	1	DRY
	Chloroform	67-66-3	N	INITIAL	ug/Kg		U		1.37	1.37	3.33	N	Y	1	DRY
	Chloromethane	74-87-3	N	INITIAL	ug/Kg		U		5.79	5.79	16.6	N	Y	1	DRY
	cis-1,2-Dichloroethene	156-59-2	N	INITIAL	ug/Kg		U		0.978	0.978	3.33	N	Y	1	DRY
	cis-1,3-Dichloropropene	10061-01-5	N	INITIAL	ug/Kg		U		1.01	1.01	3.33	N	Y	1	DRY
	Dibromomethane	74-95-3	N	INITIAL	ug/Kg		U		0.999	0.999	6.66	N	Y	1	DRY
	Dichlorodifluoromethane	75-71-8	N	INITIAL	ug/Kg		U		2.14	2.14	6.66	N	Y	1	DRY
	Di-isopropyl ether	108-20-3	N	INITIAL	ug/Kg		U		0.546	0.546	1.33	N	Y	1	DRY
	Hexachloro-1,3-butadiene	87-68-3	N	INITIAL	ug/Kg		U		7.99	7.99	33.3	N	Y	1	DRY
	Isopropylbenzene	98-82-8	N	INITIAL	ug/Kg		U		0.566	0.566	3.33	N	Y	1	DRY
	Methyl tert-butyl ether	1634-04-4	N	INITIAL	ug/Kg		U		0.466	0.466	1.33	N	Y	1	DRY
	Methylene Chloride	75-09-2	N	INITIAL	ug/Kg		U		8.84	8.84	33.3	N	Y	1	DRY
	n-Butylbenzene	104-51-8	N	INITIAL	ug/Kg		U		6.99	6.99	16.6	N	Y	1	DRY
	n-Propylbenzene	103-65-1	N	INITIAL	ug/Kg		U		1.27	1.27	6.66	N	Y	1	DRY
	p-Isopropyltoluene	99-87-6	N	INITIAL	ug/Kg		U		3.40	3.40	6.66	N	Y	1	DRY

Lab Sample ID	L1853786-01
Sys Sample Code	GACO0430T031S007
Sample Name	GACO0430T031S007
Sample Date	4/30/2025 3:35:00 PM
Sample Type	N
Matrix	SO
Parent Sample	
% Moisture	14.20

Analytic Method	Chemical Name	CAS Rn	Fraction	Test Type	Result Unit	Final Result	Final Qual	Reason code	Final MDL	Final RL	Final QL	Final Detect	Final Report	DF	Basis
SW8260	sec-Butylbenzene	135-98-8	N	INITIAL	ug/Kg		U		3.84	3.84	16.6	N	Y	1	DRY
	Styrene	100-42-5	N	INITIAL	ug/Kg		U		0.305	0.305	16.6	N	Y	1	DRY
	tert-Butylbenzene	98-06-6	N	INITIAL	ug/Kg		U		2.60	2.60	6.66	N	Y	1	DRY
	Tetrachloroethene	127-18-4	N	INITIAL	ug/Kg		U		1.19	1.19	3.33	N	Y	1	DRY
	trans-1,2-Dichloroethene	156-60-5	N	INITIAL	ug/Kg		U		1.39	1.39	6.66	N	Y	1	DRY
	trans-1,3-Dichloropropene	10061-02-6	N	INITIAL	ug/Kg		U		1.52	1.52	6.66	N	Y	1	DRY
	Trichloroethene	79-01-6	N	INITIAL	ug/Kg		U		0.778	0.778	1.33	N	Y	1	DRY
	Trichlorofluoromethane	75-69-4	N	INITIAL	ug/Kg		U		1.10	1.10	3.33	N	Y	1	DRY
SW8270	Vinyl chloride	75-01-4	N	INITIAL	ug/Kg		U		1.55	1.55	3.33	N	Y	1	DRY
	1,2,4-Trichlorobenzene	120-82-1	N	INITIAL	ug/Kg		U		24.2	24.2	776	N	Y	2	DRY
	1,2-Dichlorobenzene	95-50-1	N	INITIAL	ug/Kg		U		23.0	23.0	776	N	Y	2	DRY
	1,3-Dichlorobenzene	541-73-1	N	INITIAL	ug/Kg		U		23.5	23.5	776	N	Y	2	DRY
	1,4-Dichlorobenzene	106-46-7	N	INITIAL	ug/Kg		U		23.1	23.1	776	N	Y	2	DRY
	2,2-Oxybis(1-Chloropropane)	108-60-1	N	INITIAL	ug/Kg		U		33.6	33.6	776	N	Y	2	DRY
	2,4,6-Trichlorophenol	88-06-2	N	INITIAL	ug/Kg		U		24.9	24.9	776	N	Y	2	DRY
	2,4-Dichlorophenol	120-83-2	N	INITIAL	ug/Kg		U		22.6	22.6	776	N	Y	2	DRY
	2,4-Dimethylphenol	105-67-9	N	INITIAL	ug/Kg		U		20.3	20.3	776	N	Y	2	DRY
	2,4-Dinitrophenol	51-28-5	N	INITIAL	ug/Kg		U		182	182	776	N	Y	2	DRY
	2,4-Dinitrotoluene	121-14-2	N	INITIAL	ug/Kg		U		22.3	22.3	776	N	Y	2	DRY
	2,6-Dinitrotoluene	606-20-2	N	INITIAL	ug/Kg		U		25.4	25.4	776	N	Y	2	DRY
	2-Chloronaphthalene	91-58-7	N	INITIAL	ug/Kg		U		13.6	13.6	77.6	N	Y	2	DRY
	2-Chlorophenol	95-57-8	N	INITIAL	ug/Kg		U		25.6	25.6	776	N	Y	2	DRY
	2-Nitrophenol	88-75-5	N	INITIAL	ug/Kg		U		27.7	27.7	776	N	Y	2	DRY
	3,3-Dichlorobenzidine	91-94-1	N	INITIAL	ug/Kg		U		28.7	28.7	776	N	Y	2	DRY
	4,6-Dinitro-2-methylphenol	534-52-1	N	INITIAL	ug/Kg		U		176	176	776	N	Y	2	DRY
	4-Bromophenyl-phenylether	101-55-3	N	INITIAL	ug/Kg		U		27.3	27.3	776	N	Y	2	DRY
	4-Chloro-3-methylphenol	59-50-7	N	INITIAL	ug/Kg		U		25.2	25.2	776	N	Y	2	DRY
	4-Chlorophenyl-phenylether	7005-72-3	N	INITIAL	ug/Kg		U		27.0	27.0	776	N	Y	2	DRY
	4-Nitrophenol	100-02-7	N	INITIAL	ug/Kg		U		24.2	24.2	776	N	Y	2	DRY
	Acenaphthylene	208-96-8	N	INITIAL	ug/Kg		U		10.9	10.9	77.6	N	Y	2	DRY
	Benzidine	92-87-5	N	INITIAL	ug/Kg		U		146	146	3890	N	Y	2	DRY
	Benzo(g,h,i)perylene	191-24-2	N	INITIAL	ug/Kg		U		14.2	14.2	77.6	N	Y	2	DRY
Benzylbutyl phthalate	85-68-7	N	INITIAL	ug/Kg		U		24.2	24.2	776	N	Y	2	DRY	

Lab Sample ID	L1853786-01
Sys Sample Code	GACO0430T031S007
Sample Name	GACO0430T031S007
Sample Date	4/30/2025 3:35:00 PM
Sample Type	N
Matrix	SO
Parent Sample	
% Moisture	14.20

Analytic Method	Chemical Name	CAS Rn	Fraction	Test Type	Result Unit	Final Result	Final Qual	Reason code	Final MDL	Final RL	Final QL	Final Detect	Final Report	DF	Basis
SW8270	Bis(2-chlorethoxy)methane	111-91-1	N	INITIAL	ug/Kg		U		23.3	23.3	776	N	Y	2	DRY
	Bis(2-chloroethyl)ether	111-44-4	N	INITIAL	ug/Kg		U		25.6	25.6	776	N	Y	2	DRY
	Bis(2-ethylhexyl)phthalate	117-81-7	N	INITIAL	ug/Kg		U		98.4	98.4	776	N	Y	2	DRY
	Diethyl phthalate	84-66-2	N	INITIAL	ug/Kg		U		25.6	25.6	776	N	Y	2	DRY
	Dimethyl phthalate	131-11-3	N	INITIAL	ug/Kg		U		164	164	776	N	Y	2	DRY
	Di-n-butyl phthalate	84-74-2	N	INITIAL	ug/Kg		U		26.6	26.6	776	N	Y	2	DRY
	Di-n-octyl phthalate	117-84-0	N	INITIAL	ug/Kg		U		52.5	52.5	776	N	Y	2	DRY
	Hexachloro-1,3-butadiene	87-68-3	N	INITIAL	ug/Kg		U		26.1	26.1	776	N	Y	2	DRY
	Hexachlorobenzene	118-74-1	N	INITIAL	ug/Kg		U		27.5	27.5	776	N	Y	2	DRY
	Hexachlorocyclopentadiene	77-47-4	N	INITIAL	ug/Kg		R	MS-	40.8	40.8	776	N	Y	2	DRY
	Hexachloroethane	67-72-1	N	INITIAL	ug/Kg		U		30.5	30.5	776	N	Y	2	DRY
	Isophorone	78-59-1	N	INITIAL	ug/Kg		U		23.8	23.8	776	N	Y	2	DRY
	Nitrobenzene	98-95-3	N	INITIAL	ug/Kg		U		27.0	27.0	776	N	Y	2	DRY
	n-Nitrosodimethylamine	62-75-9	N	INITIAL	ug/Kg		U		115	115	776	N	Y	2	DRY
	n-Nitrosodi-n-propylamine	621-64-7	N	INITIAL	ug/Kg		U		25.9	25.9	776	N	Y	2	DRY
	n-Nitrosodiphenylamine	86-30-6	N	INITIAL	ug/Kg		U		58.8	58.8	776	N	Y	2	DRY
	Pentachlorophenol	87-86-5	N	INITIAL	ug/Kg		U		20.9	20.9	776	N	Y	2	DRY
	Phenanthrene	85-01-8	N	INITIAL	ug/Kg		U		15.4	15.4	77.6	N	Y	2	DRY
Phenol	108-95-2	N	INITIAL	ug/Kg		U		31.2	31.2	776	N	Y	2	DRY	
SW9056	Nitrate-Nitrite	NO2-NO3	N	INITIAL	ug/Kg	68900			706	706	23300	Y	Y	1	DRY
WBLACK	TOC By Walkley Black	10-35-5	N	INITIAL	ug/Kg	35600000			230000	230000	900000	Y	Y	9	NA

Lab Sample ID	L1853786-02
Sys Sample Code	GACO0430T031S006
Sample Name	GACO0430T031S006
Sample Date	4/30/2025 3:30:00 PM
Sample Type	N
Matrix	SO
Parent Sample	
% Moisture	12.90

Analytic Method	Chemical Name	CAS Rn	Fraction	Test Type	Result Unit	Final Result	Final Qual	Reason code	Final MDL	Final RL	Final QL	Final Detect	Final Report	DF	Basis
CALC	Total Nitrogen	TN	N	INITIAL	ug/Kg	1540000			696	696	23000	Y	Y	1	DRY
E350.1	Ammonia Nitrogen	7664-41-7	N	INITIAL	ug/Kg		U		8250	8250	11500	N	Y	1	DRY
SM2540G	Total Solids	10-31-1	N	INITIAL	%	87.1						Y	Y	1	NA
SM4500-NORG-D	Kjeldahl Nitrogen, TKN	7727-37-9TKN	N	INITIAL	ug/Kg	1490000			174000	174000	230000	Y	Y	10	DRY
SW6010	Aluminum	7429-90-5	T	INITIAL	ug/Kg	2380000	J	MS,MSP	6980	6980	23000	Y	Y	1	DRY
	Antimony	7440-36-0	T	INITIAL	ug/Kg		U		793	793	2300	N	Y	1	DRY
	Beryllium	7440-41-7	T	INITIAL	ug/Kg	418			54.8	54.8	230	Y	Y	1	DRY
	Calcium	7440-70-2	T	INITIAL	ug/Kg	4470000			21800	21800	115000	Y	Y	1	DRY
	Cobalt	7440-48-4	T	INITIAL	ug/Kg	4400			203	203	1150	Y	Y	1	DRY
	Iron	7439-89-6	T	INITIAL	ug/Kg	2800000	J-	MS-	2570	2570	11500	Y	Y	1	DRY
	Magnesium	7439-95-4	T	INITIAL	ug/Kg	1510000			22800	22800	115000	Y	Y	1	DRY
	Manganese	7439-96-5	T	INITIAL	ug/Kg	213000	J-	MS-	199	199	1150	Y	Y	1	DRY
	Potassium	7440-09-7	T	INITIAL	ug/Kg	1860000			24000	24000	115000	Y	Y	1	DRY
	Sodium	7440-23-5	T	INITIAL	ug/Kg	144000			47300	47300	115000	Y	Y	1	DRY
	Thallium	7440-28-0	T	INITIAL	ug/Kg			U		595	595	2300	N	Y	1
Vanadium	7440-62-2	T	INITIAL	ug/Kg	8850			440	440	2300	Y	Y	1	DRY	
SW8260	1,1,1,2-Tetrachloroethane	630-20-6	N	INITIAL	ug/Kg		U		1.23	1.23	3.24	N	Y	1	DRY
	1,1,1-Trichloroethane	71-55-6	N	INITIAL	ug/Kg		U		1.20	1.20	3.24	N	Y	1	DRY
	1,1,2,2-Tetrachloroethane	79-34-5	N	INITIAL	ug/Kg		U		0.900	0.900	3.24	N	Y	1	DRY
	1,1,2-Trichloroethane	79-00-5	N	INITIAL	ug/Kg		U		0.774	0.774	3.24	N	Y	1	DRY
	1,1,2-Trichlorotrifluoroethane	76-13-1	N	INITIAL	ug/Kg		U		0.977	0.977	3.24	N	Y	1	DRY
	1,1-Dichloroethane	75-34-3	N	INITIAL	ug/Kg		U		0.636	0.636	3.24	N	Y	1	DRY
	1,1-Dichloroethene	75-35-4	N	INITIAL	ug/Kg		U		0.785	0.785	3.24	N	Y	1	DRY
	1,1-Dichloropropene	563-58-6	N	INITIAL	ug/Kg		U		1.05	1.05	3.24	N	Y	1	DRY
	1,2,3-Trichlorobenzene	87-61-6	N	INITIAL	ug/Kg		U		9.50	9.50	16.2	N	Y	1	DRY
	1,2,3-Trichloropropane	96-18-4	N	INITIAL	ug/Kg		U		2.10	2.10	16.2	N	Y	1	DRY
	1,2,3-Trimethylbenzene	526-73-8	N	INITIAL	ug/Kg		U		2.05	2.05	6.48	N	Y	1	DRY
	1,2,4-Trichlorobenzene	120-82-1	N	INITIAL	ug/Kg		U		5.70	5.70	16.2	N	Y	1	DRY
	1,2-Dibromo-3-Chloropropane	96-12-8	N	INITIAL	ug/Kg		U		5.05	5.05	32.4	N	Y	1	DRY
	1,2-Dibromoethane	106-93-4	N	INITIAL	ug/Kg		U		0.840	0.840	3.24	N	Y	1	DRY
	1,2-Dichlorobenzene	95-50-1	N	INITIAL	ug/Kg		U		0.551	0.551	6.48	N	Y	1	DRY
	1,2-Dichloroethane	107-06-2	N	INITIAL	ug/Kg		U		0.841	0.841	3.24	N	Y	1	DRY

Lab Sample ID	L1853786-02
Sys Sample Code	GACO0430T031S006
Sample Name	GACO0430T031S006
Sample Date	4/30/2025 3:30:00 PM
Sample Type	N
Matrix	SO
Parent Sample	
% Moisture	12.90

Analytic Method	Chemical Name	CAS Rn	Fraction	Test Type	Result Unit	Final Result	Final Qual	Reason code	Final MDL	Final RL	Final QL	Final Detect	Final Report	DF	Basis
SW8260	1,2-Dichloropropane	78-87-5	N	INITIAL	ug/Kg		U		1.84	1.84	6.48	N	Y	1	DRY
	1,3-Dichlorobenzene	541-73-1	N	INITIAL	ug/Kg		U		0.777	0.777	6.48	N	Y	1	DRY
	1,3-Dichloropropane	142-28-9	N	INITIAL	ug/Kg		U		0.649	0.649	6.48	N	Y	1	DRY
	1,4-Dichlorobenzene	106-46-7	N	INITIAL	ug/Kg		U		0.907	0.907	6.48	N	Y	1	DRY
	2,2-Dichloropropane	594-20-7	N	INITIAL	ug/Kg		U		1.79	1.79	3.24	N	Y	1	DRY
	2-Butanone (MEK)	78-93-3	N	INITIAL	ug/Kg		U		82.3	82.3	130	N	Y	1	DRY
	2-Chlorotoluene	95-49-8	N	INITIAL	ug/Kg		U		1.12	1.12	3.24	N	Y	1	DRY
	4-Chlorotoluene	106-43-4	N	INITIAL	ug/Kg		U		0.583	0.583	6.48	N	Y	1	DRY
	4-Methyl-2-pentanone (MIBK)	108-10-1	N	INITIAL	ug/Kg		U		2.95	2.95	32.4	N	Y	1	DRY
	Acetone	67-64-1	N	INITIAL	ug/Kg		U		47.3	47.3	64.8	N	Y	1	DRY
	Acrylonitrile	107-13-1	N	INITIAL	ug/Kg		U		4.68	4.68	16.2	N	Y	1	DRY
	Bromobenzene	108-86-1	N	INITIAL	ug/Kg		U		1.17	1.17	16.2	N	Y	1	DRY
	Bromodichloromethane	75-27-4	N	INITIAL	ug/Kg		U		0.939	0.939	3.24	N	Y	1	DRY
	Bromoform	75-25-2	N	INITIAL	ug/Kg		U		1.52	1.52	32.4	N	Y	1	DRY
	Bromomethane	74-83-9	N	INITIAL	ug/Kg		U		2.55	2.55	16.2	N	Y	1	DRY
	Carbon tetrachloride	56-23-5	N	INITIAL	ug/Kg		U		1.16	1.16	6.48	N	Y	1	DRY
	Chlorobenzene	108-90-7	N	INITIAL	ug/Kg		U		0.272	0.272	3.24	N	Y	1	DRY
	Chlorodibromomethane	124-48-1	N	INITIAL	ug/Kg		U		0.793	0.793	3.24	N	Y	1	DRY
	Chloroethane	75-00-3	N	INITIAL	ug/Kg		U		2.20	2.20	6.48	N	Y	1	DRY
	Chloroform	67-66-3	N	INITIAL	ug/Kg		U		1.33	1.33	3.24	N	Y	1	DRY
	Chloromethane	74-87-3	N	INITIAL	ug/Kg		U		5.64	5.64	16.2	N	Y	1	DRY
	cis-1,2-Dichloroethene	156-59-2	N	INITIAL	ug/Kg		U		0.951	0.951	3.24	N	Y	1	DRY
	cis-1,3-Dichloropropene	10061-01-5	N	INITIAL	ug/Kg		U		0.981	0.981	3.24	N	Y	1	DRY
	Dibromomethane	74-95-3	N	INITIAL	ug/Kg		U		0.972	0.972	6.48	N	Y	1	DRY
	Dichlorodifluoromethane	75-71-8	N	INITIAL	ug/Kg		U		2.09	2.09	6.48	N	Y	1	DRY
	Di-isopropyl ether	108-20-3	N	INITIAL	ug/Kg		U		0.531	0.531	1.30	N	Y	1	DRY
	Hexachloro-1,3-butadiene	87-68-3	N	INITIAL	ug/Kg		U		7.77	7.77	32.4	N	Y	1	DRY
	Isopropylbenzene	98-82-8	N	INITIAL	ug/Kg		U		0.551	0.551	3.24	N	Y	1	DRY
	Methyl tert-butyl ether	1634-04-4	N	INITIAL	ug/Kg		U		0.453	0.453	1.30	N	Y	1	DRY
	Methylene Chloride	75-09-2	N	INITIAL	ug/Kg		U		8.60	8.60	32.4	N	Y	1	DRY
	n-Butylbenzene	104-51-8	N	INITIAL	ug/Kg		U		6.80	6.80	16.2	N	Y	1	DRY
	n-Propylbenzene	103-65-1	N	INITIAL	ug/Kg		U		1.23	1.23	6.48	N	Y	1	DRY
	p-Isopropyltoluene	99-87-6	N	INITIAL	ug/Kg		U		3.30	3.30	6.48	N	Y	1	DRY

Lab Sample ID	L1853786-02
Sys Sample Code	GACO0430T031S006
Sample Name	GACO0430T031S006
Sample Date	4/30/2025 3:30:00 PM
Sample Type	N
Matrix	SO
Parent Sample	
% Moisture	12.90

Analytic Method	Chemical Name	CAS Rn	Fraction	Test Type	Result Unit	Final Result	Final Qual	Reason code	Final MDL	Final RL	Final QL	Final Detect	Final Report	DF	Basis
SW8260	sec-Butylbenzene	135-98-8	N	INITIAL	ug/Kg		U		3.73	3.73	16.2	N	Y	1	DRY
	Styrene	100-42-5	N	INITIAL	ug/Kg		U		0.297	0.297	16.2	N	Y	1	DRY
	tert-Butylbenzene	98-06-6	N	INITIAL	ug/Kg		U		2.53	2.53	6.48	N	Y	1	DRY
	Tetrachloroethene	127-18-4	N	INITIAL	ug/Kg		U		1.16	1.16	3.24	N	Y	1	DRY
	trans-1,2-Dichloroethene	156-60-5	N	INITIAL	ug/Kg		U		1.35	1.35	6.48	N	Y	1	DRY
	trans-1,3-Dichloropropene	10061-02-6	N	INITIAL	ug/Kg		U		1.48	1.48	6.48	N	Y	1	DRY
	Trichloroethene	79-01-6	N	INITIAL	ug/Kg		U		0.757	0.757	1.30	N	Y	1	DRY
	Trichlorofluoromethane	75-69-4	N	INITIAL	ug/Kg		U		1.07	1.07	3.24	N	Y	1	DRY
	Vinyl chloride	75-01-4	N	INITIAL	ug/Kg		U		1.50	1.50	3.24	N	Y	1	DRY
SW8270	1,2,4-Trichlorobenzene	120-82-1	N	INITIAL	ug/Kg		U		23.9	23.9	764	N	Y	2	DRY
	1,2-Dichlorobenzene	95-50-1	N	INITIAL	ug/Kg		U		22.6	22.6	764	N	Y	2	DRY
	1,3-Dichlorobenzene	541-73-1	N	INITIAL	ug/Kg		U		23.2	23.2	764	N	Y	2	DRY
	1,4-Dichlorobenzene	106-46-7	N	INITIAL	ug/Kg		U		22.7	22.7	764	N	Y	2	DRY
	2,2-Oxybis(1-Chloropropane)	108-60-1	N	INITIAL	ug/Kg		U		33.1	33.1	764	N	Y	2	DRY
	2,4,6-Trichlorophenol	88-06-2	N	INITIAL	ug/Kg		U		24.6	24.6	764	N	Y	2	DRY
	2,4-Dichlorophenol	120-83-2	N	INITIAL	ug/Kg		U		22.3	22.3	764	N	Y	2	DRY
	2,4-Dimethylphenol	105-67-9	N	INITIAL	ug/Kg		U		20.0	20.0	764	N	Y	2	DRY
	2,4-Dinitrophenol	51-28-5	N	INITIAL	ug/Kg		U		179	179	764	N	Y	2	DRY
	2,4-Dinitrotoluene	121-14-2	N	INITIAL	ug/Kg		U		21.9	21.9	764	N	Y	2	DRY
	2,6-Dinitrotoluene	606-20-2	N	INITIAL	ug/Kg		U		25.0	25.0	764	N	Y	2	DRY
	2-Chloronaphthalene	91-58-7	N	INITIAL	ug/Kg		U		13.4	13.4	76.4	N	Y	2	DRY
	2-Chlorophenol	95-57-8	N	INITIAL	ug/Kg		U		25.3	25.3	764	N	Y	2	DRY
	2-Nitrophenol	88-75-5	N	INITIAL	ug/Kg		U		27.3	27.3	764	N	Y	2	DRY
	3,3-Dichlorobenzidine	91-94-1	N	INITIAL	ug/Kg		U		28.2	28.2	764	N	Y	2	DRY
	4,6-Dinitro-2-methylphenol	534-52-1	N	INITIAL	ug/Kg		U		173	173	764	N	Y	2	DRY
	4-Bromophenyl-phenylether	101-55-3	N	INITIAL	ug/Kg		U		26.9	26.9	764	N	Y	2	DRY
	4-Chloro-3-methylphenol	59-50-7	N	INITIAL	ug/Kg		U		24.8	24.8	764	N	Y	2	DRY
	4-Chlorophenyl-phenylether	7005-72-3	N	INITIAL	ug/Kg		U		26.6	26.6	764	N	Y	2	DRY
	4-Nitrophenol	100-02-7	N	INITIAL	ug/Kg		U		23.9	23.9	764	N	Y	2	DRY
Acenaphthylene	208-96-8	N	INITIAL	ug/Kg		U		10.8	10.8	76.4	N	Y	2	DRY	
Benzidine	92-87-5	N	INITIAL	ug/Kg		U		143	143	3830	N	Y	2	DRY	
Benzo(g,h,i)perylene	191-24-2	N	INITIAL	ug/Kg		U		14.0	14.0	76.4	N	Y	2	DRY	
Benzylbutyl phthalate	85-68-7	N	INITIAL	ug/Kg		U		23.9	23.9	764	N	Y	2	DRY	

Lab Sample ID	L1853786-02
Sys Sample Code	GACO0430T031S006
Sample Name	GACO0430T031S006
Sample Date	4/30/2025 3:30:00 PM
Sample Type	N
Matrix	SO
Parent Sample	
% Moisture	12.90

Analytic Method	Chemical Name	CAS Rn	Fraction	Test Type	Result Unit	Final Result	Final Qual	Reason code	Final MDL	Final RL	Final QL	Final Detect	Final Report	DF	Basis
SW8270	Bis(2-chlorethoxy)methane	111-91-1	N	INITIAL	ug/Kg		U		23.0	23.0	764	N	Y	2	DRY
	Bis(2-chloroethyl)ether	111-44-4	N	INITIAL	ug/Kg		U		25.3	25.3	764	N	Y	2	DRY
	Bis(2-ethylhexyl)phthalate	117-81-7	N	INITIAL	ug/Kg		U		96.9	96.9	764	N	Y	2	DRY
	Diethyl phthalate	84-66-2	N	INITIAL	ug/Kg		U		25.3	25.3	764	N	Y	2	DRY
	Dimethyl phthalate	131-11-3	N	INITIAL	ug/Kg		U		162	162	764	N	Y	2	DRY
	Di-n-butyl phthalate	84-74-2	N	INITIAL	ug/Kg		U		26.2	26.2	764	N	Y	2	DRY
	Di-n-octyl phthalate	117-84-0	N	INITIAL	ug/Kg		U		51.7	51.7	764	N	Y	2	DRY
	Hexachloro-1,3-butadiene	87-68-3	N	INITIAL	ug/Kg		U		25.7	25.7	764	N	Y	2	DRY
	Hexachlorobenzene	118-74-1	N	INITIAL	ug/Kg		U		27.1	27.1	764	N	Y	2	DRY
	Hexachlorocyclopentadiene	77-47-4	N	INITIAL	ug/Kg		U		40.2	40.2	764	N	Y	2	DRY
	Hexachloroethane	67-72-1	N	INITIAL	ug/Kg		U		30.1	30.1	764	N	Y	2	DRY
	Isophorone	78-59-1	N	INITIAL	ug/Kg		U		23.4	23.4	764	N	Y	2	DRY
	Nitrobenzene	98-95-3	N	INITIAL	ug/Kg		U		26.6	26.6	764	N	Y	2	DRY
	n-Nitrosodimethylamine	62-75-9	N	INITIAL	ug/Kg		U		113	113	764	N	Y	2	DRY
	n-Nitrosodi-n-propylamine	621-64-7	N	INITIAL	ug/Kg		U		25.5	25.5	764	N	Y	2	DRY
	n-Nitrosodiphenylamine	86-30-6	N	INITIAL	ug/Kg		U		57.9	57.9	764	N	Y	2	DRY
	Pentachlorophenol	87-86-5	N	INITIAL	ug/Kg		U		20.5	20.5	764	N	Y	2	DRY
	Phenanthrene	85-01-8	N	INITIAL	ug/Kg		U		15.2	15.2	76.4	N	Y	2	DRY
Phenol	108-95-2	N	INITIAL	ug/Kg		U		30.8	30.8	764	N	Y	2	DRY	
SW9056	Nitrate-Nitrite	NO2-NO3	N	INITIAL	ug/Kg	43100			696	696	23000	Y	Y	1	DRY
WBLACK	TOC By Walkley Black	10-35-5	N	INITIAL	ug/Kg	17400000			128000	128000	500000	Y	Y	5	NA

Lab Sample ID	L1853786-03
Sys Sample Code	GACO0430T031S005
Sample Name	GACO0430T031S005
Sample Date	4/30/2025 11:25:00 AM
Sample Type	N
Matrix	SO
Parent Sample	
% Moisture	70.80

Analytic Method	Chemical Name	CAS Rn	Fraction	Test Type	Result Unit	Final Result	Final Qual	Reason code	Final MDL	Final RL	Final QL	Final Detect	Final Report	DF	Basis
CALC	Total Nitrogen	TN	N	INITIAL	ug/Kg	24000000			10400	10400	343000	Y	Y	1	DRY
E350.1	Ammonia Nitrogen	7664-41-7	N	INITIAL	ug/Kg		U		24600	24600	34300	N	Y	1	DRY
SM2540G	Total Solids	10-31-1	N	INITIAL	%	29.2						Y	Y	1	NA
SM4500-NORG-D	Kjeldahl Nitrogen, TKN	7727-37-9TKN	N	INITIAL	ug/Kg	23600000			1040000	1040000	1370000	Y	Y	20	DRY
SW6010	Aluminum	7429-90-5	T	INITIAL	ug/Kg	1810000	J	MS,MSP	20800	20800	68500	Y	Y	1	DRY
	Antimony	7440-36-0	T	INITIAL	ug/Kg		U		2370	2370	6850	N	Y	1	DRY
	Beryllium	7440-41-7	T	INITIAL	ug/Kg	375	J	RL	163	163	685	Y	Y	1	DRY
	Calcium	7440-70-2	T	INITIAL	ug/Kg	26300000			65100	65100	343000	Y	Y	1	DRY
	Cobalt	7440-48-4	T	INITIAL	ug/Kg	4310			606	606	3430	Y	Y	1	DRY
	Iron	7439-89-6	T	INITIAL	ug/Kg	5290000	J-	MS-	7670	7670	34300	Y	Y	1	DRY
	Magnesium	7439-95-4	T	INITIAL	ug/Kg	4070000			68200	68200	343000	Y	Y	1	DRY
	Manganese	7439-96-5	T	INITIAL	ug/Kg	440000	J-	MS-	593	593	3430	Y	Y	1	DRY
	Potassium	7440-09-7	T	INITIAL	ug/Kg	6050000			71600	71600	343000	Y	Y	1	DRY
	Sodium	7440-23-5	T	INITIAL	ug/Kg	3270000			141000	141000	343000	Y	Y	1	DRY
	Thallium	7440-28-0	T	INITIAL	ug/Kg			U	1770	1770	6850	N	Y	1	DRY
Vanadium	7440-62-2	T	INITIAL	ug/Kg	10100			1310	1310	6850	Y	Y	1	DRY	
SW8260	1,1,1,2-Tetrachloroethane	630-20-6	N	INITIAL	ug/Kg		U		11.1	11.1	29.3	N	Y	2	DRY
	1,1,1-Trichloroethane	71-55-6	N	INITIAL	ug/Kg		U		10.8	10.8	29.3	N	Y	2	DRY
	1,1,2,2-Tetrachloroethane	79-34-5	N	INITIAL	ug/Kg		U		8.14	8.14	29.3	N	Y	2	DRY
	1,1,2-Trichloroethane	79-00-5	N	INITIAL	ug/Kg		U		6.97	6.97	29.3	N	Y	2	DRY
	1,1,2-Trichlorotrifluoroethane	76-13-1	N	INITIAL	ug/Kg		U		8.84	8.84	29.3	N	Y	2	DRY
	1,1-Dichloroethane	75-34-3	N	INITIAL	ug/Kg		U		5.75	5.75	29.3	N	Y	2	DRY
	1,1-Dichloroethene	75-35-4	N	INITIAL	ug/Kg		U		7.09	7.09	29.3	N	Y	2	DRY
	1,1-Dichloropropene	563-58-6	N	INITIAL	ug/Kg		U		9.49	9.49	29.3	N	Y	2	DRY
	1,2,3-Trichlorobenzene	87-61-6	N	INITIAL	ug/Kg		U		86.1	86.1	146	N	Y	2	DRY
	1,2,3-Trichloropropane	96-18-4	N	INITIAL	ug/Kg		U		19.0	19.0	146	N	Y	2	DRY
	1,2,3-Trimethylbenzene	526-73-8	N	INITIAL	ug/Kg		U		18.5	18.5	58.6	N	Y	2	DRY
	1,2,4-Trichlorobenzene	120-82-1	N	INITIAL	ug/Kg		U		51.5	51.5	146	N	Y	2	DRY
	1,2-Dibromo-3-Chloropropane	96-12-8	N	INITIAL	ug/Kg		U		45.7	45.7	293	N	Y	2	DRY
	1,2-Dibromoethane	106-93-4	N	INITIAL	ug/Kg		U		7.61	7.61	29.3	N	Y	2	DRY
	1,2-Dichlorobenzene	95-50-1	N	INITIAL	ug/Kg		U		4.98	4.98	58.6	N	Y	2	DRY
	1,2-Dichloroethane	107-06-2	N	INITIAL	ug/Kg		U		7.61	7.61	29.3	N	Y	2	DRY

Lab Sample ID	L1853786-03
Sys Sample Code	GACO0430T031S005
Sample Name	GACO0430T031S005
Sample Date	4/30/2025 11:25:00 AM
Sample Type	N
Matrix	SO
Parent Sample	
% Moisture	70.80

Analytic Method	Chemical Name	CAS Rn	Fraction	Test Type	Result Unit	Final Result	Final Qual	Reason code	Final MDL	Final RL	Final QL	Final Detect	Final Report	DF	Basis
SW8260	1,2-Dichloropropane	78-87-5	N	INITIAL	ug/Kg		U		16.6	16.6	58.6	N	Y	2	DRY
	1,3-Dichlorobenzene	541-73-1	N	INITIAL	ug/Kg		U		7.03	7.03	58.6	N	Y	2	DRY
	1,3-Dichloropropane	142-28-9	N	INITIAL	ug/Kg		U		5.86	5.86	58.6	N	Y	2	DRY
	1,4-Dichlorobenzene	106-46-7	N	INITIAL	ug/Kg		U		8.20	8.20	58.6	N	Y	2	DRY
	2,2-Dichloropropane	594-20-7	N	INITIAL	ug/Kg		U		16.2	16.2	29.3	N	Y	2	DRY
	2-Butanone (MEK)	78-93-3	N	INITIAL	ug/Kg		U		744	744	1170	N	Y	2	DRY
	2-Chlorotoluene	95-49-8	N	INITIAL	ug/Kg		U		10.1	10.1	29.3	N	Y	2	DRY
	4-Chlorotoluene	106-43-4	N	INITIAL	ug/Kg		U		5.27	5.27	58.6	N	Y	2	DRY
	4-Methyl-2-pentanone (MIBK)	108-10-1	N	INITIAL	ug/Kg		U		26.7	26.7	293	N	Y	2	DRY
	Acetone	67-64-1	N	INITIAL	ug/Kg		U		428	428	586	N	Y	2	DRY
	Acrylonitrile	107-13-1	N	INITIAL	ug/Kg		U		42.3	42.3	146	N	Y	2	DRY
	Bromobenzene	108-86-1	N	INITIAL	ug/Kg		U		10.5	10.5	146	N	Y	2	DRY
	Bromodichloromethane	75-27-4	N	INITIAL	ug/Kg		U		8.49	8.49	29.3	N	Y	2	DRY
	Bromoform	75-25-2	N	INITIAL	ug/Kg		U		13.7	13.7	293	N	Y	2	DRY
	Bromomethane	74-83-9	N	INITIAL	ug/Kg		U		23.1	23.1	146	N	Y	2	DRY
	Carbon tetrachloride	56-23-5	N	INITIAL	ug/Kg		U		10.5	10.5	58.6	N	Y	2	DRY
	Chlorobenzene	108-90-7	N	INITIAL	ug/Kg		U		2.46	2.46	29.3	N	Y	2	DRY
	Chlorodibromomethane	124-48-1	N	INITIAL	ug/Kg		U		7.15	7.15	29.3	N	Y	2	DRY
	Chloroethane	75-00-3	N	INITIAL	ug/Kg		U		19.9	19.9	58.6	N	Y	2	DRY
	Chloroform	67-66-3	N	INITIAL	ug/Kg		U		12.1	12.1	29.3	N	Y	2	DRY
	Chloromethane	74-87-3	N	INITIAL	ug/Kg		U		51.0	51.0	146	N	Y	2	DRY
	cis-1,2-Dichloroethene	156-59-2	N	INITIAL	ug/Kg		U		8.61	8.61	29.3	N	Y	2	DRY
	cis-1,3-Dichloropropene	10061-01-5	N	INITIAL	ug/Kg		U		8.84	8.84	29.3	N	Y	2	DRY
	Dibromomethane	74-95-3	N	INITIAL	ug/Kg		U		8.79	8.79	58.6	N	Y	2	DRY
	Dichlorodifluoromethane	75-71-8	N	INITIAL	ug/Kg		U		18.9	18.9	58.6	N	Y	2	DRY
	Di-isopropyl ether	108-20-3	N	INITIAL	ug/Kg		U		4.80	4.80	11.7	N	Y	2	DRY
	Hexachloro-1,3-butadiene	87-68-3	N	INITIAL	ug/Kg		U		70.3	70.3	293	N	Y	2	DRY
	Isopropylbenzene	98-82-8	N	INITIAL	ug/Kg		U		4.98	4.98	29.3	N	Y	2	DRY
	Methyl tert-butyl ether	1634-04-4	N	INITIAL	ug/Kg		U		4.10	4.10	11.7	N	Y	2	DRY
	Methylene Chloride	75-09-2	N	INITIAL	ug/Kg		U		77.9	77.9	293	N	Y	2	DRY
	n-Butylbenzene	104-51-8	N	INITIAL	ug/Kg		U		61.5	61.5	146	N	Y	2	DRY
	n-Propylbenzene	103-65-1	N	INITIAL	ug/Kg		U		11.1	11.1	58.6	N	Y	2	DRY
	p-Isopropyltoluene	99-87-6	N	INITIAL	ug/Kg		U		29.9	29.9	58.6	N	Y	2	DRY

Lab Sample ID	L1853786-03
Sys Sample Code	GACO0430T031S005
Sample Name	GACO0430T031S005
Sample Date	4/30/2025 11:25:00 AM
Sample Type	N
Matrix	SO
Parent Sample	
% Moisture	70.80

Analytic Method	Chemical Name	CAS Rn	Fraction	Test Type	Result Unit	Final Result	Final Qual	Reason code	Final MDL	Final RL	Final QL	Final Detect	Final Report	DF	Basis
SW8260	sec-Butylbenzene	135-98-8	N	INITIAL	ug/Kg		U		33.7	33.7	146	N	Y	2	DRY
	Styrene	100-42-5	N	INITIAL	ug/Kg		U		2.68	2.68	146	N	Y	2	DRY
	tert-Butylbenzene	98-06-6	N	INITIAL	ug/Kg		U		22.8	22.8	58.6	N	Y	2	DRY
	Tetrachloroethene	127-18-4	N	INITIAL	ug/Kg		U		10.5	10.5	29.3	N	Y	2	DRY
	trans-1,2-Dichloroethene	156-60-5	N	INITIAL	ug/Kg		U		12.2	12.2	58.6	N	Y	2	DRY
	trans-1,3-Dichloropropene	10061-02-6	N	INITIAL	ug/Kg		U		13.4	13.4	58.6	N	Y	2	DRY
	Trichloroethene	79-01-6	N	INITIAL	ug/Kg		U		6.85	6.85	11.7	N	Y	2	DRY
	Trichlorofluoromethane	75-69-4	N	INITIAL	ug/Kg		U		9.66	9.66	29.3	N	Y	2	DRY
	Vinyl chloride	75-01-4	N	INITIAL	ug/Kg		U		13.6	13.6	29.3	N	Y	2	DRY
SW8270	1,2,4-Trichlorobenzene	120-82-1	N	INITIAL	ug/Kg		U		713	713	22800	N	Y	20	DRY
	1,2-Dichlorobenzene	95-50-1	N	INITIAL	ug/Kg		U		675	675	22800	N	Y	20	DRY
	1,3-Dichlorobenzene	541-73-1	N	INITIAL	ug/Kg		U		692	692	22800	N	Y	20	DRY
	1,4-Dichlorobenzene	106-46-7	N	INITIAL	ug/Kg		U		678	678	22800	N	Y	20	DRY
	2,2-Oxybis(1-Chloropropane)	108-60-1	N	INITIAL	ug/Kg		U		987	987	22800	N	Y	20	DRY
	2,4,6-Trichlorophenol	88-06-2	N	INITIAL	ug/Kg		U		733	733	22800	N	Y	20	DRY
	2,4-Dichlorophenol	120-83-2	N	INITIAL	ug/Kg		U		665	665	22800	N	Y	20	DRY
	2,4-Dimethylphenol	105-67-9	N	INITIAL	ug/Kg		U		596	596	22800	N	Y	20	DRY
	2,4-Dinitrophenol	51-28-5	N	INITIAL	ug/Kg		U		5340	5340	22800	N	Y	20	DRY
	2,4-Dinitrotoluene	121-14-2	N	INITIAL	ug/Kg		U		654	654	22800	N	Y	20	DRY
	2,6-Dinitrotoluene	606-20-2	N	INITIAL	ug/Kg		U		747	747	22800	N	Y	20	DRY
	2-Chloronaphthalene	91-58-7	N	INITIAL	ug/Kg		U		401	401	2280	N	Y	20	DRY
	2-Chlorophenol	95-57-8	N	INITIAL	ug/Kg		U		754	754	22800	N	Y	20	DRY
	2-Nitrophenol	88-75-5	N	INITIAL	ug/Kg		U		815	815	22800	N	Y	20	DRY
	3,3-Dichlorobenzidine	91-94-1	N	INITIAL	ug/Kg		U		843	843	22800	N	Y	20	DRY
	4,6-Dinitro-2-methylphenol	534-52-1	N	INITIAL	ug/Kg		U		5170	5170	22800	N	Y	20	DRY
	4-Bromophenyl-phenylether	101-55-3	N	INITIAL	ug/Kg		U		802	802	22800	N	Y	20	DRY
	4-Chloro-3-methylphenol	59-50-7	N	INITIAL	ug/Kg		U		740	740	22800	N	Y	20	DRY
	4-Chlorophenyl-phenylether	7005-72-3	N	INITIAL	ug/Kg		U		795	795	22800	N	Y	20	DRY
	4-Nitrophenol	100-02-7	N	INITIAL	ug/Kg		U		713	713	22800	N	Y	20	DRY
	Acenaphthylene	208-96-8	N	INITIAL	ug/Kg		U		321	321	2280	N	Y	20	DRY
Benzidine	92-87-5	N	INITIAL	ug/Kg		U		4280	4280	114000	N	Y	20	DRY	
Benzo(g,h,i)perylene	191-24-2	N	INITIAL	ug/Kg		U		418	418	2280	N	Y	20	DRY	
Benzylbutyl phthalate	85-68-7	N	INITIAL	ug/Kg		U		713	713	22800	N	Y	20	DRY	

Lab Sample ID	L1853786-03
Sys Sample Code	GACO0430T031S005
Sample Name	GACO0430T031S005
Sample Date	4/30/2025 11:25:00 AM
Sample Type	N
Matrix	SO
Parent Sample	
% Moisture	70.80

Analytic Method	Chemical Name	CAS Rn	Fraction	Test Type	Result Unit	Final Result	Final Qual	Reason code	Final MDL	Final RL	Final QL	Final Detect	Final Report	DF	Basis
SW8270	Bis(2-chlorethoxy)methane	111-91-1	N	INITIAL	ug/Kg		U		685	685	22800	N	Y	20	DRY
	Bis(2-chloroethyl)ether	111-44-4	N	INITIAL	ug/Kg		U		754	754	22800	N	Y	20	DRY
	Bis(2-ethylhexyl)phthalate	117-81-7	N	INITIAL	ug/Kg		U		2890	2890	22800	N	Y	20	DRY
	Diethyl phthalate	84-66-2	N	INITIAL	ug/Kg		U		754	754	22800	N	Y	20	DRY
	Dimethyl phthalate	131-11-3	N	INITIAL	ug/Kg		U		4830	4830	22800	N	Y	20	DRY
	Di-n-butyl phthalate	84-74-2	N	INITIAL	ug/Kg		U		781	781	22800	N	Y	20	DRY
	Di-n-octyl phthalate	117-84-0	N	INITIAL	ug/Kg		U		1540	1540	22800	N	Y	20	DRY
	Hexachloro-1,3-butadiene	87-68-3	N	INITIAL	ug/Kg		U		767	767	22800	N	Y	20	DRY
	Hexachlorobenzene	118-74-1	N	INITIAL	ug/Kg		U		809	809	22800	N	Y	20	DRY
	Hexachlorocyclopentadiene	77-47-4	N	INITIAL	ug/Kg		U		1200	1200	22800	N	Y	20	DRY
	Hexachloroethane	67-72-1	N	INITIAL	ug/Kg		U		898	898	22800	N	Y	20	DRY
	Isophorone	78-59-1	N	INITIAL	ug/Kg		U		699	699	22800	N	Y	20	DRY
	Nitrobenzene	98-95-3	N	INITIAL	ug/Kg		U		795	795	22800	N	Y	20	DRY
	n-Nitrosodimethylamine	62-75-9	N	INITIAL	ug/Kg		U		3380	3380	22800	N	Y	20	DRY
	n-Nitrosodi-n-propylamine	621-64-7	N	INITIAL	ug/Kg		U		761	761	22800	N	Y	20	DRY
	n-Nitrosodiphenylamine	86-30-6	N	INITIAL	ug/Kg		U		1730	1730	22800	N	Y	20	DRY
	Pentachlorophenol	87-86-5	N	INITIAL	ug/Kg		U		613	613	22800	N	Y	20	DRY
	Phenanthrene	85-01-8	N	INITIAL	ug/Kg		U		452	452	2280	N	Y	20	DRY
Phenol	108-95-2	N	INITIAL	ug/Kg		U		918	918	22800	N	Y	20	DRY	
SW9056	Nitrate-Nitrite	NO2-NO3	N	INITIAL	ug/Kg	445000			10400	10400	343000	Y	Y	5	DRY
WBLACK	TOC By Walkley Black	10-35-5	N	INITIAL	ug/Kg	92500000			434000	434000	1700000	Y	Y	17	NA

Lab Sample ID	L1853786-04
Sys Sample Code	GACO0430T031T002
Sample Name	GACO0430T031T002
Sample Date	4/30/2025 7:00:00 AM
Sample Type	TB
Matrix	WQ
Parent Sample	
% Moisture	

Analytic Method	Chemical Name	CAS Rn	Fraction	Test Type	Result Unit	Final Result	Final Qual	Reason code	Final MDL	Final RL	Final QL	Final Detect	Final Report	DF	Basis
SW8260	1,1,1,2-Tetrachloroethane	630-20-6	N	INITIAL	ug/L		U		0.147	0.147	1.00	N	Y	1	NA
	1,1,1-Trichloroethane	71-55-6	N	INITIAL	ug/L		U		0.149	0.149	1.00	N	Y	1	NA
	1,1,2,2-Tetrachloroethane	79-34-5	N	INITIAL	ug/L		U		0.133	0.133	1.00	N	Y	1	NA
	1,1,2-Trichloroethane	79-00-5	N	INITIAL	ug/L		U		0.158	0.158	1.00	N	Y	1	NA
	1,1,2-Trichlorotrifluoroethane	76-13-1	N	INITIAL	ug/L		U		0.180	0.180	1.00	N	Y	1	NA
	1,1-Dichloroethane	75-34-3	N	INITIAL	ug/L		U		0.100	0.100	1.00	N	Y	1	NA
	1,1-Dichloroethene	75-35-4	N	INITIAL	ug/L		U		0.188	0.188	1.00	N	Y	1	NA
	1,1-Dichloropropene	563-58-6	N	INITIAL	ug/L		U		0.142	0.142	1.00	N	Y	1	NA
	1,2,3-Trichlorobenzene	87-61-6	N	INITIAL	ug/L		U		0.230	0.230	1.00	N	Y	1	NA
	1,2,3-Trichloropropane	96-18-4	N	INITIAL	ug/L		U		0.237	0.237	2.50	N	Y	1	NA
	1,2,3-Trimethylbenzene	526-73-8	N	INITIAL	ug/L		U		0.104	0.104	1.00	N	Y	1	NA
	1,2,4-Trichlorobenzene	120-82-1	N	INITIAL	ug/L		U		0.481	0.481	1.00	N	Y	1	NA
	1,2,4-Trimethylbenzene	95-63-6	N	INITIAL	ug/L		U		0.322	0.322	1.00	N	Y	1	NA
	1,2-Dibromo-3-Chloropropane	96-12-8	N	INITIAL	ug/L		U		0.276	0.276	5.00	N	Y	1	NA
	1,2-Dibromoethane	106-93-4	N	INITIAL	ug/L		U		0.126	0.126	1.00	N	Y	1	NA
	1,2-Dichlorobenzene	95-50-1	N	INITIAL	ug/L		U		0.107	0.107	1.00	N	Y	1	NA
	1,2-Dichloroethane	107-06-2	N	INITIAL	ug/L		R	LC-	0.0819	0.0819	1.00	N	Y	1	NA
	1,2-Dichloropropane	78-87-5	N	INITIAL	ug/L		U		0.149	0.149	1.00	N	Y	1	NA
	1,3,5-Trimethylbenzene	108-67-8	N	INITIAL	ug/L		U		0.104	0.104	1.00	N	Y	1	NA
	1,3-Dichlorobenzene	541-73-1	N	INITIAL	ug/L		U		0.110	0.110	1.00	N	Y	1	NA
	1,3-Dichloropropane	142-28-9	N	INITIAL	ug/L		U		0.110	0.110	1.00	N	Y	1	NA
	1,4-Dichlorobenzene	106-46-7	N	INITIAL	ug/L		U		0.120	0.120	1.00	N	Y	1	NA
	2,2-Dichloropropane	594-20-7	N	INITIAL	ug/L		U		0.161	0.161	1.00	N	Y	1	NA
	2-Butanone (MEK)	78-93-3	N	INITIAL	ug/L		U		1.19	1.19	10.0	N	Y	1	NA
	2-Chlorotoluene	95-49-8	N	INITIAL	ug/L		U		0.106	0.106	1.00	N	Y	1	NA
	4-Chlorotoluene	106-43-4	N	INITIAL	ug/L		U		0.114	0.114	1.00	N	Y	1	NA
	4-Methyl-2-pentanone (MIBK)	108-10-1	N	INITIAL	ug/L		U		0.478	0.478	10.0	N	Y	1	NA
	Acetone	67-64-1	N	INITIAL	ug/L		U		11.3	11.3	50.0	N	Y	1	NA
	Acrolein	107-02-8	N	INITIAL	ug/L		U		2.54	2.54	50.0	N	Y	1	NA
	Acrylonitrile	107-13-1	N	INITIAL	ug/L		U		0.671	0.671	10.0	N	Y	1	NA
	Benzene	71-43-2	N	INITIAL	ug/L		U		0.0941	0.0941	1.00	N	Y	1	NA
	Bromobenzene	108-86-1	N	INITIAL	ug/L		U		0.118	0.118	1.00	N	Y	1	NA
	Bromodichloromethane	75-27-4	N	INITIAL	ug/L		U		0.136	0.136	1.00	N	Y	1	NA

Lab Sample ID	L1853786-04
Sys Sample Code	GACO0430T031T002
Sample Name	GACO0430T031T002
Sample Date	4/30/2025 7:00:00 AM
Sample Type	TB
Matrix	WQ
Parent Sample	
% Moisture	

Analytic Method	Chemical Name	CAS Rn	Fraction	Test Type	Result Unit	Final Result	Final Qual	Reason code	Final MDL	Final RL	Final QL	Final Detect	Final Report	DF	Basis
SW8260	Bromoform	75-25-2	N	INITIAL	ug/L		U		0.129	0.129	1.00	N	Y	1	NA
	Bromomethane	74-83-9	N	INITIAL	ug/L		U		0.605	0.605	5.00	N	Y	1	NA
	Carbon tetrachloride	56-23-5	N	INITIAL	ug/L		U		0.128	0.128	1.00	N	Y	1	NA
	Chlorobenzene	108-90-7	N	INITIAL	ug/L		U		0.116	0.116	1.00	N	Y	1	NA
	Chlorodibromomethane	124-48-1	N	INITIAL	ug/L		U		0.140	0.140	1.00	N	Y	1	NA
	Chloroethane	75-00-3	N	INITIAL	ug/L		U		0.192	0.192	5.00	N	Y	1	NA
	Chloroform	67-66-3	N	INITIAL	ug/L		U		0.111	0.111	5.00	N	Y	1	NA
	Chloromethane	74-87-3	N	INITIAL	ug/L		U		0.960	0.960	2.50	N	Y	1	NA
	cis-1,2-Dichloroethene	156-59-2	N	INITIAL	ug/L		U		0.126	0.126	1.00	N	Y	1	NA
	cis-1,3-Dichloropropene	10061-01-5	N	INITIAL	ug/L		U		0.111	0.111	1.00	N	Y	1	NA
	Dibromomethane	74-95-3	N	INITIAL	ug/L		U		0.122	0.122	1.00	N	Y	1	NA
	Dichlorodifluoromethane	75-71-8	N	INITIAL	ug/L		U		0.374	0.374	5.00	N	Y	1	NA
	Di-isopropyl ether	108-20-3	N	INITIAL	ug/L		U		0.105	0.105	1.00	N	Y	1	NA
	Ethylbenzene	100-41-4	N	INITIAL	ug/L		U		0.137	0.137	1.00	N	Y	1	NA
	Hexachloro-1,3-butadiene	87-68-3	N	INITIAL	ug/L		U		0.337	0.337	1.00	N	Y	1	NA
	Isopropylbenzene	98-82-8	N	INITIAL	ug/L		U		0.105	0.105	1.00	N	Y	1	NA
	Methyl tert-butyl ether	1634-04-4	N	INITIAL	ug/L		U		0.101	0.101	1.00	N	Y	1	NA
	Methylene Chloride	75-09-2	N	INITIAL	ug/L		U		0.430	0.430	5.00	N	Y	1	NA
	Naphthalene	91-20-3	N	INITIAL	ug/L		U		1.00	1.00	5.00	N	Y	1	NA
	n-Butylbenzene	104-51-8	N	INITIAL	ug/L		U		0.157	0.157	1.00	N	Y	1	NA
	n-Propylbenzene	103-65-1	N	INITIAL	ug/L		U		0.0993	0.0993	1.00	N	Y	1	NA
	p-Isopropyltoluene	99-87-6	N	INITIAL	ug/L		U		0.120	0.120	1.00	N	Y	1	NA
	sec-Butylbenzene	135-98-8	N	INITIAL	ug/L		U		0.125	0.125	1.00	N	Y	1	NA
	Styrene	100-42-5	N	INITIAL	ug/L		U		0.118	0.118	1.00	N	Y	1	NA
	tert-Butylbenzene	98-06-6	N	INITIAL	ug/L		U		0.127	0.127	1.00	N	Y	1	NA
	Tetrachloroethene	127-18-4	N	INITIAL	ug/L		U		0.300	0.300	1.00	N	Y	1	NA
	Toluene	108-88-3	N	INITIAL	ug/L		U		0.278	0.278	1.00	N	Y	1	NA
	trans-1,2-Dichloroethene	156-60-5	N	INITIAL	ug/L		U		0.149	0.149	1.00	N	Y	1	NA
	trans-1,3-Dichloropropene	10061-02-6	N	INITIAL	ug/L		U		0.118	0.118	1.00	N	Y	1	NA
	Trichloroethene	79-01-6	N	INITIAL	ug/L		U		0.190	0.190	1.00	N	Y	1	NA
Trichlorofluoromethane	75-69-4	N	INITIAL	ug/L		U		0.160	0.160	5.00	N	Y	1	NA	
Vinyl chloride	75-01-4	N	INITIAL	ug/L		U		0.234	0.234	1.00	N	Y	1	NA	
Xylenes, Total	1330-20-7	N	INITIAL	ug/L		U		0.174	0.174	3.00	N	Y	1	NA	